



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA100) Micron Test Report

Oasis Acres, LLC/L. Benton/R. & D. Fowler
3131 S. Duck Lake Road
Highland MI 48356-3333 USA

08/23/19

Test No: 981590

Animal and Sample Description


Animal Name: OA"s XXXTreme Daredevil XXX
Breed: Alpaca(Huacaya)
Sex: Male
Color: Lt Brown

Animal ID: 35589334
Sample Location: Side
Sample Date: 05/04/19
Age: 08/15/18

Laboratory Data

Mean Fiber Diameter: 16.7 microns
Standard Deviation: 4.1 microns
Coefficient of Variation: 24.6 %
Fibers Greater Than 30 microns: 1.3 %

Spin Fineness: 16.7 microns
Medullated Fibers: 0.0 %
Mean Curvature (deg/mm): 57.2
SD Curvature (deg/mm): 30.5

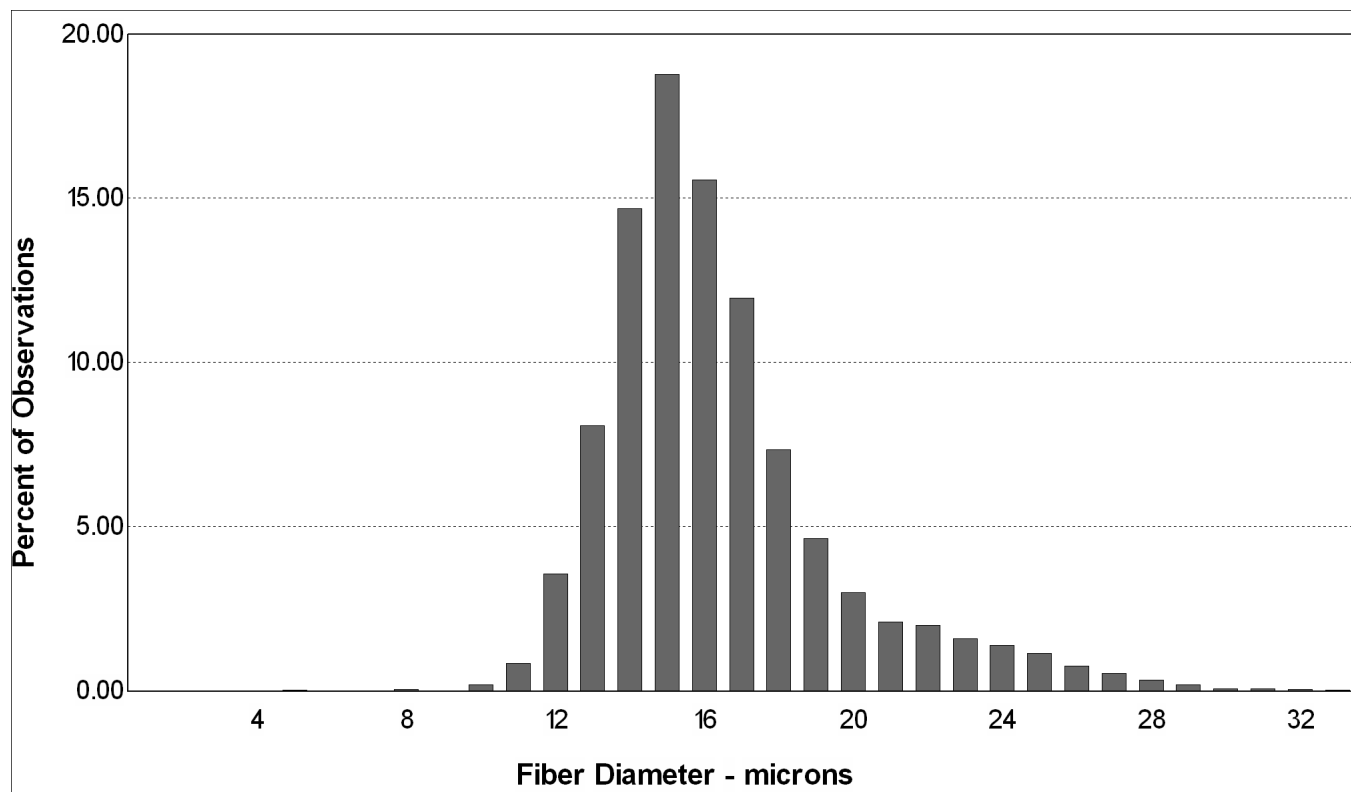

This Test Performed According to I.W.T.O Method 47