



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA100) Micron Test Report

Oasis Acres, LLC/L. Benton/R. & D. Fowler
3131 S. Duck Lake Road
Highland MI 48356-3333 USA

08/23/19

Test No: 981591


Animal and Sample Description

Animal Name: OA"s Lady Liberty XX
Breed: Alpaca(Huacaya)
Sex: Female
Color: Lt Brown

Animal ID: 35589389
Sample Location: Side
Sample Date: 05/04/19
Age: 06/16/18

Laboratory Data

Mean Fiber Diameter:	16.4 microns	Spin Fineness:	16.1 microns
Standard Deviation:	3.6 microns	Medullated Fibers:	0.0 %
Coefficient of Variation:	21.9 %	Mean Curvature (deg/mm):	46.0
Fibers Greater Than 30 microns:	0.9 %	SD Curvature (deg/mm):	24.4

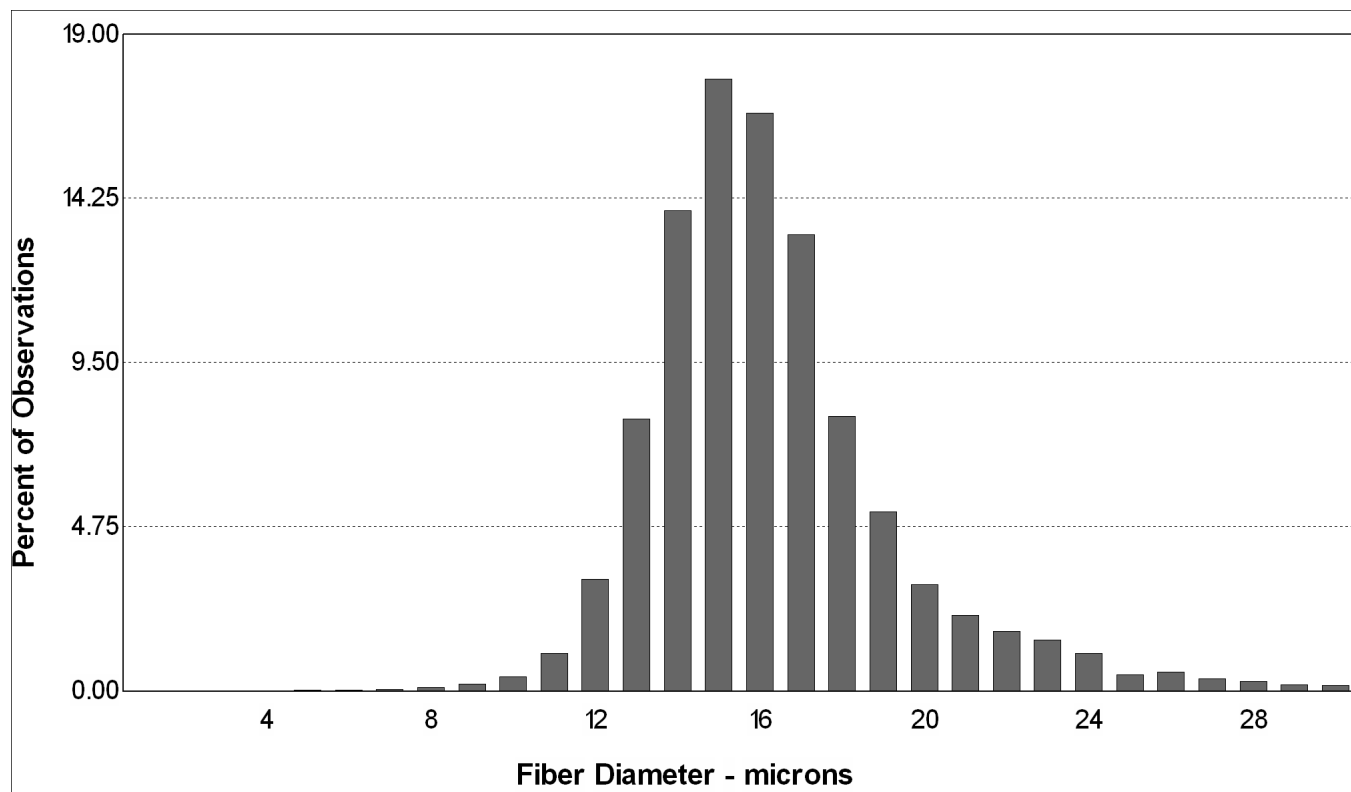

This Test Performed According to I.W.T.O Method 47